


MASS SPECTROMETRY REPORT

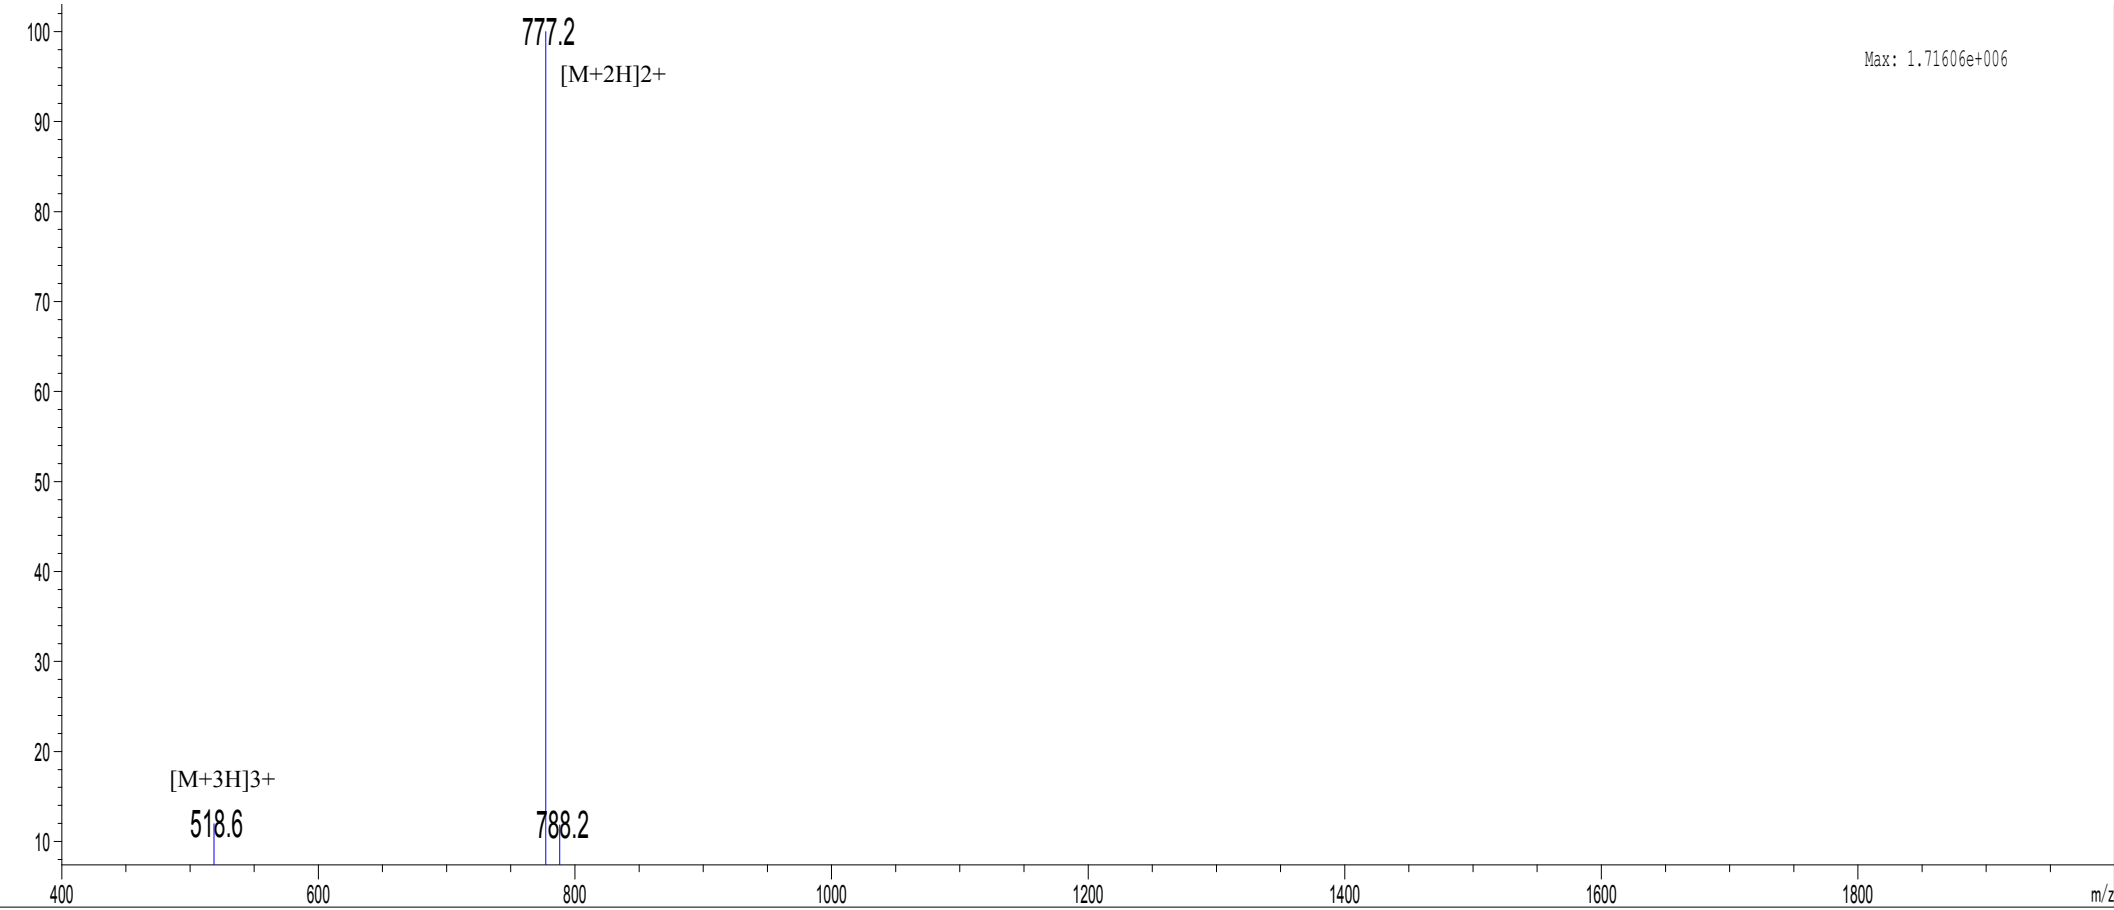

Sample Description		Instrument		Agilent-6125B	
Analyzed date:	2025-07-11	Probe:	ESI	Probe Bias:	+4.5kv
Analyst:	YU	Nebulizer Gas Flow:	1.5L/min	Detector:	1.5kv
Sample:	同位素标记猪 I 型 GR-18	CDL:	-20.0v	T. Flow:	0.2ml/min
M.W.:	1552.68	CDL Temp.:	250 °C	B. Conc.:	50%H2O/50%ACN
Lot. No.:	P250627-SJ1271770	Block Temp.:	200 °C		